


PLATELET FUNCTION ASSESSMENT

WITH THE SONOCLOT® COAGULATION & PLATELET FUNCTION ANALYZER


CHARACTERIZE CLOT RETRACTION WITH THE gbACT+ TEST

- Whole Blood Platelet Function Assessment
- Platelet Function and ACT Results in One Test
- Results Typically in 15 Minutes
- Automated Platelet Function Results with Signature Viewer™*

ASSESS PLATELET FUNCTION

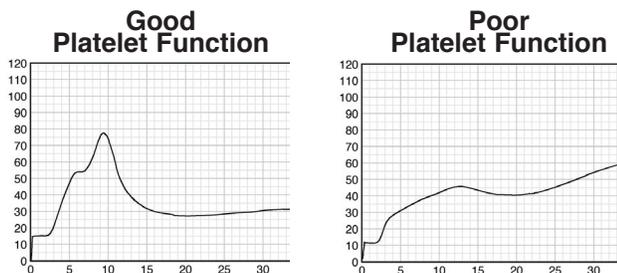


MANAGE BLOOD PRODUCTS

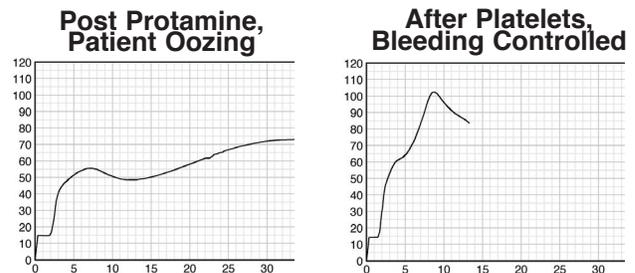


EVALUATE RESPONSE TO PLATELET GP II_bIII_a INHIBITORS

Eptifibatide Dose Response

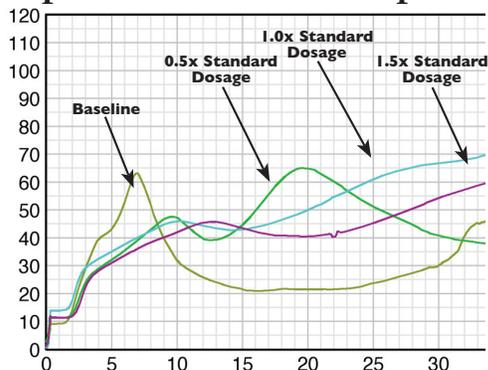

ReoPro™ Dose Response

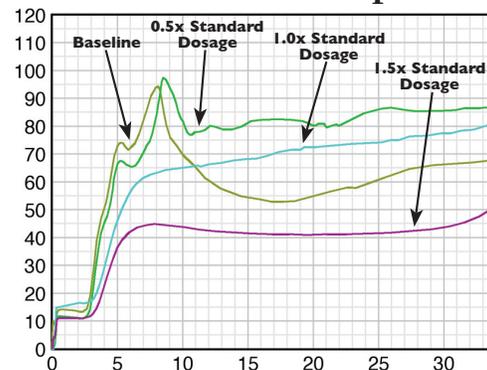

* Quantitative Results with Sonoclot® Analyzer and Signature Viewer Software, Qualitative Results with Sonoclot® Analyzer Connected to Graphics Printer